



**INFECTION
CONTROL**®

July/August 1981

Volume 2/Number 4

Editorial

**Infection Control in Perspective: Infections
Due to Medical Equipment and Devices**

William M. Valenti, M.D.

Original Articles

**Ordering Patterns, Collection, Transport, and
Screening of Sputum Cultures in a Community Hospital:
Evaluation of Methods to Improve Results**

Julie T. Jacobson, B.S., M.T. (ASCP); John P. Burke, M.D.;
and Jay A. Jacobson, M.D.

**Recurrent Meningococcal Meningitis Caused by Poly
Groups X-W135: Importance of Chemoprophylaxis**

Richard F. Jacobs, M.D. and Terry Yamauchi, M.D.

**Bacteriologic Studies on Electronic
Hospital Thermometers**

Leon Smith, M.D.; Herbert N. Prince, Ph.D.;
and Edward Johnson, M.D.

**Toxocariasis in an Institution for the
Mentally Retarded**

Itzhak Brook, M.D., M.S.; Charles H. Fish, M.D., M.P.H.;
Peter N. Schantz, V.M.D., Ph.D.; and David D. Cotton, M.D.


BARD ANNOUNCES

bn-74
CATHETER COATING™

AN ADVANCEMENT
IN THE FIGHT AGAINST
NOSOCOMIAL URINARY
TRACT INFECTION

Available Exclusively on the bn-74
Coated BARDEX® All Silicone Foley Catheter

A NEW TECHNOLOGY now offers a
barrier to bacterial migration by providing
a surface on a Foley Catheter which
effectively absorbs antimicro-
bial solutions.

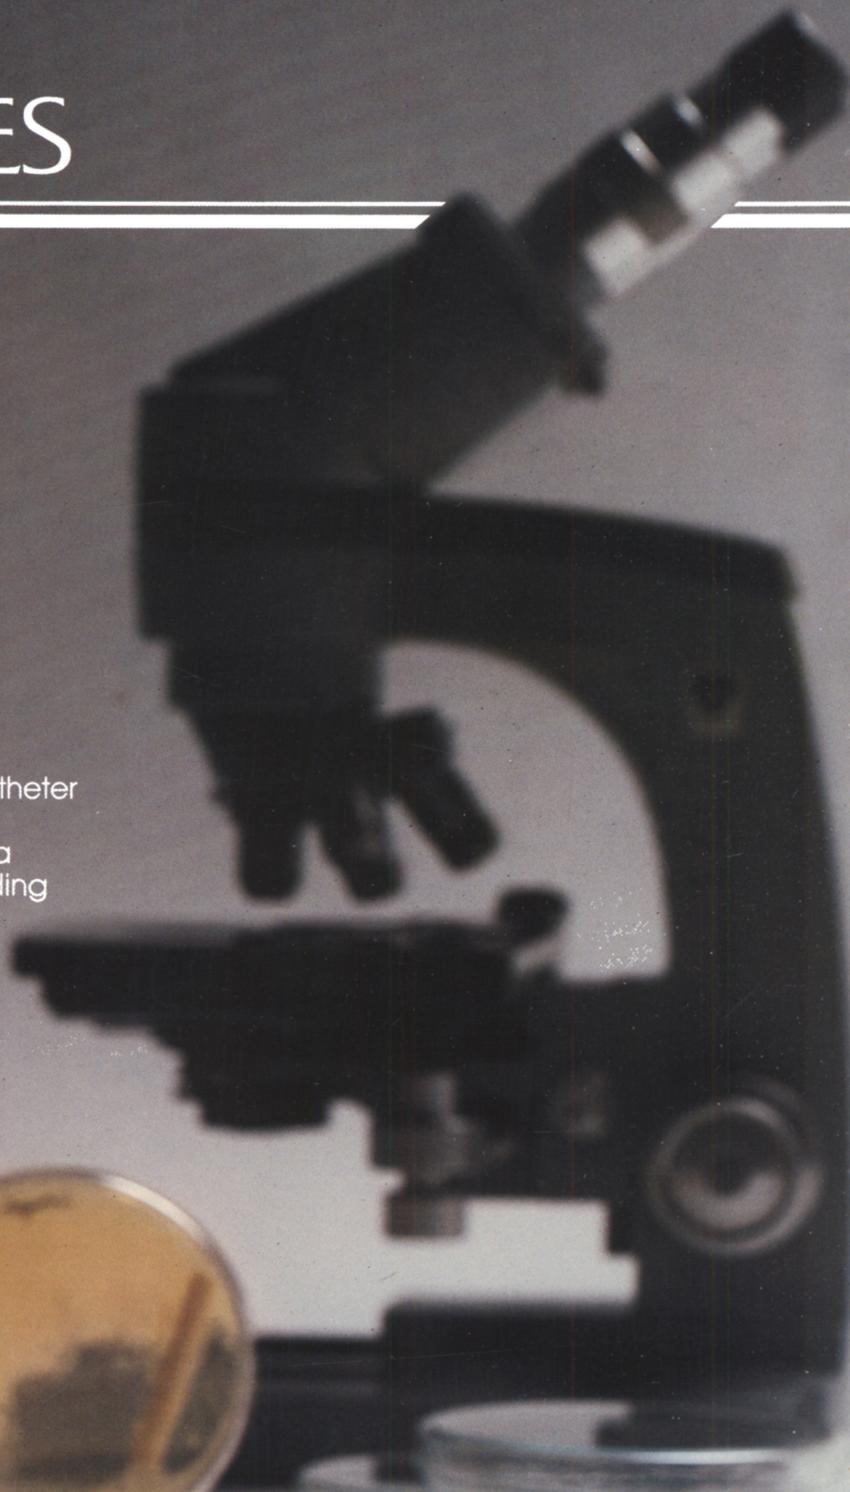

THE ONLY FOLEY CATHETER WITH THESE INFECTION CONTROL FEATURES



IT'S WETTABLE

Absorbs antimicrobial solutions into catheter surface to aid in reducing bacterial migration

A. bn-74™ Coated Catheter section:

Unique hydrophilic nature of bn-74 Coating allows povidone-iodine to absorb into the catheter surface

B. Hydrophobic surfaces of uncoated catheter sections: Povidone-iodine beads and rolls off uncoated latex or silicone catheters



IT RESISTS STATIC BUILDUP

C. The bn-74 hydrophilic surface reduces static electricity, minimizing attraction of particulate matter—another aid in infection control

D. Static electricity on hydrophobic surfaces of uncoated silicone catheters can attract pathogen-containing dust or lint, creating an additional infection hazard

THE bn-74 CONTRIBUTION TO INFECTION CONTROL

Because bn-74 absorbs antimicrobial solutions, it is now technically feasible to prepare a bactericidal surface on the catheter shaft surface at a potential site of contamination...After insertion, the catheter is coated with an antimicrobial solution from where it enters the meatus to the catheter bifurcation. In laboratory testing bn-74 coated catheters and uncoated sections were treated with an antimicrobial solution and then exposed to *Staphylococcus aureus* and *Escherichia coli*. The results showed effectiveness of the absorbed antimicrobial solution on the bn-74 coated catheter against the bacteria being tested.

bn-74
CATHETER COATING™

COATED BARDEX®
ALL SILICONE FOLEY
CATHETER


AN ADVANCEMENT
IN CATHETER COATING...
A CONTRIBUTION TO
INFECTION CONTROL

ONLY FROM BARD...
EXCLUSIVE COMPONENTS IN A UNIQUE
SYSTEM FOR INFECTION CONTROL

bn-74
CATHETER COATING™

**COATED BARDEX® ALL
SILICONE FOLEY CATHETER**

- Absorbs antimicrobial solutions to help minimize bacterial migration
- Resists static buildup to further aid in infection control

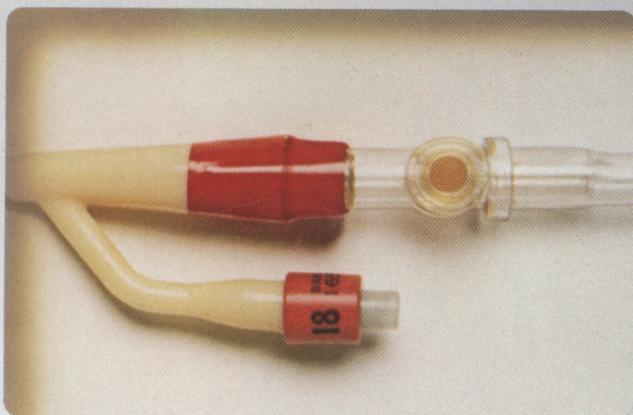


EXCLUSIVE BARD® TAMPER EVIDENT SEAL*
Helps provide a continuous, unbroken catheter/
drainage tube linkup

- prevents accidental disconnection of catheter connector
- discourages intentional disconnection
- provides visual evidence of a break in the closed system

**The bn-74 Coated BARDEX®
All Silicone Foley Catheter**
Available in a tray with complete components
for sterile catheterization procedure. Also
available individually and in a BARD® Bladder
Care Tray with Urine Meter Drainage Bag.



BARD® CENTER ENTRY URINARY DRAINAGE BAG
■ Limits pooling ■ Provides better balance ■ Is easier to empty

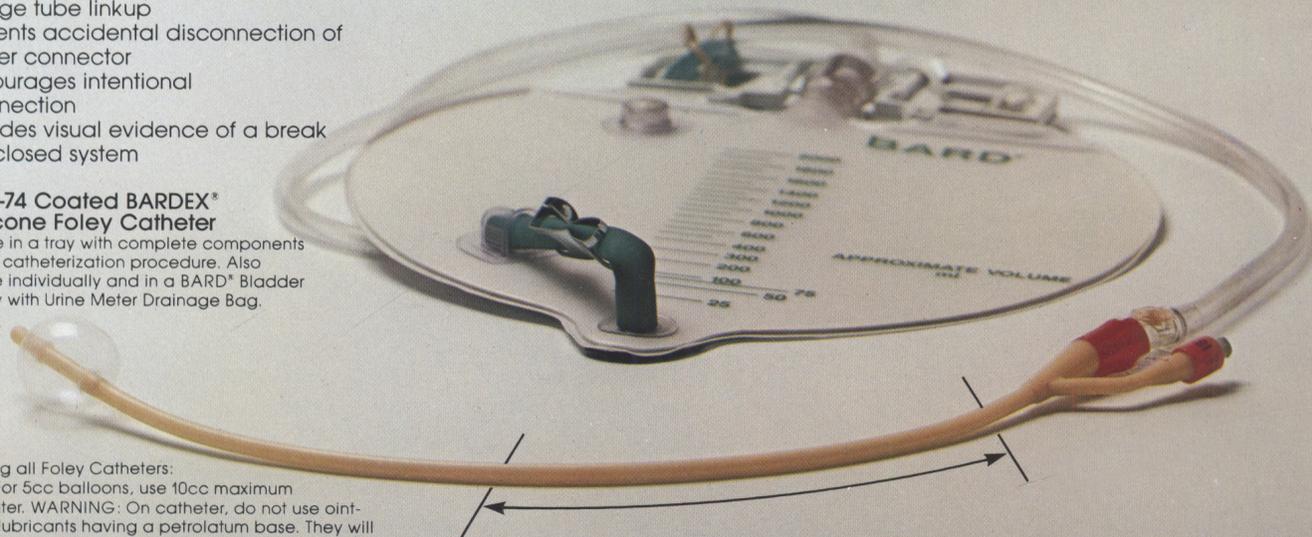

Regarding all Foley Catheters:
USAGE: For 5cc balloons, use 10cc maximum
sterile water. WARNING: On catheter, do not use oint-
ments or lubricants having a petrolatum base. They will
damage latex or silicone elastomer and may burst balloon.

Regarding all Drainage Bags and Foley Catheters:
CAUTION: Federal (U.S.A.) Law restricts these devices to
sale by or on the order of a physician.

After insertion, the antimicrobial solution is
applied to the catheter shaft from the meatus to
the bifurcation of the catheter.

BARD, BARDEX and  are trademarks registered in the
U.S. Patent and Trademark Office
by C.R. Bard, Inc.

BARD UROLOGICAL DIVISION



C.R. Bard, Inc.
Murray Hill, NJ 07974

Editorial

Infection Control in Perspective: Infections Due to Medical Equipment and Devices William M. Valenti, M.D.	305
--	-----

Original Articles

Ordering Patterns, Collection, Transport, and Screening of Sputum Cultures in a Community Hospital: Evaluation of Methods to Improve Results Julie T. Jacobson, B.S., M.T. (ASCP); John P. Burke, M.D.; and Jay A. Jacobson, M.D.	307
--	-----

Recurrent Meningococcal Meningitis Caused by Poly Groups X-W135: Importance of Chemoprophylaxis Richard F. Jacobs, M.D. and Terry Yamauchi, M.D.	312
--	-----

Bacteriologic Studies on Electronic Hospital Thermometers Leon Smith, M.D.; Herbert N. Prince, Ph.D.; and Edward Johnson, M.D.	315
---	-----

Toxocariasis in an Institution for the Mentally Retarded Itzhak Brook, M.D., M.S.; Charles H. Fish, M.D., M.P.H.; Peter M. Schantz, V.M.D., Ph.D.; and David D. Cotton, M.D.	317
---	-----

Departments

Letters to the Editor	288	Applied Statistics in IC	333
New Developments in IC	295	Index to Advertisers	337
Book Reviews	303	Legislative News	340
The Law and IC	323	Calendar of Events	344
Topics in Clinical Microbiology	327	New Products and Services	348

Publisher: Infection Control is published bimonthly by Charles B. Slack, Inc., 6900 Grove Road, Thorofare, New Jersey 08086. Telephones: Thorofare (609) 848-1000; New York (212) 285-9777.

Copyright 1981. Published bimonthly by Charles B. Slack, Inc., 6900 Grove Road, Thorofare, New Jersey 08086; telephone (609) 848-1000. All rights reserved. No part of this publication may be reproduced without written permission from the publisher.

Subscriptions: Subscription requests should be addressed to the publisher. Annual subscription price is: Individual. One year—\$22.00; Two years—\$38.00; Three years—\$54.00. Student rate: \$11.00 per year. All subscriptions, without exception, will start with the first issue published after the order is received. Back copies are available, but must be purchased separately. Cost per individual copy is \$5.00. All orders for individual issues must be accompanied by payment.

Change of address: Notice should be sent to the publisher six weeks in advance of effective date. Include old and new addresses with zip codes. The publisher cannot accept responsibility for undelivered copies. Controlled circulation postage is paid at Thorofare, New Jersey 08086.

As of Volume 1, Number 1, INFECTION CONTROL is listed in *Index Medicus*, *Current Contents—Clinical Practice*, *Hospital Literature Index*, and *Cumulative Index to Nursing and Allied Health Literature*.

Steam and Gas.

Now...SteriGage® Indicators
give you both steam and ethylene oxide
sterilization security.

Sterilization security...it's something you and your patients
receive with both the SteriGage Steam and SteriGage EO Ethylene
Oxide Sterilization Indicators.

One indicator in each load provides accurate, precise results—
no reader interpretation is necessary. And each indicator
provides instant readouts—no incubation period is required.

SteriGage and SteriGage EO...sterilization
assurance for all your needs.

For further information, call toll-free
800-631-1253, ext. 4760.

© 1981 ORGANON INC.
ORG-7182



Distributed by:
Organon Hospital Products
Organon Inc.
West Orange, NJ 07052





EDITORIAL BOARD

INFECTION CONTROL

EDITOR

Richard P. Wenzel, MD
Charlottesville, Virginia

SENIOR ASSOCIATE EDITOR

William Schaffner, MD
Nashville, Tennessee

ASSOCIATE EDITORS

Sue Crow, RN, BS, MSN
Shreveport, Louisiana

Dennis G. Maki, MD
Madison, Wisconsin

John E. McGowan, Jr., MD
Atlanta, Georgia

EDITORIAL ADVISORY BOARD

Robert C. Aber, MD
Hershey, Pennsylvania

Charles S. Bryan, MD
Columbia, South Carolina

John P. Burke, MD
Salt Lake City, Utah

Richard E. Dixon, MD
Trenton, New Jersey

Harvey A. Elder, MD
Loma Linda, California

Peter C. Fuchs, MD, PhD
Portland, Oregon

Richard A. Garibaldi, MD
Salt Lake City, Utah

Donald A. Goldmann, MD
Boston, Massachusetts

Dieter H.M. Gröschel, MD
Charlottesville, Virginia

Peter Gross, MD
Hackensack, New Jersey

Karen Hadley, RN, MPH
New Orleans, Louisiana

Cyrus C. Hopkins, MD
Boston, Massachusetts

Allen B. Kaiser, MD
Nashville, Tennessee

Harold Laufman, MD, PhD
Bronx, New York

William J. Ledger, MD
New York, New York

Barbara McArthur, RN, BSN, MS,
MS, PhD
Detroit, Michigan

Rob Roy MacGregor, MD
Philadelphia, Pennsylvania

C. Glen Mayhall, MD
Richmond, Virginia

Ronald Lee Nichols, MD
New Orleans, Louisiana

Harry C. Nottebart, Jr., JD, MD
Richmond, Virginia

Karen Paul, BS, MS
Philadelphia, Pennsylvania

Frank S. Rhame, MD
Minneapolis, Minnesota

William E. Scheckler, MD
Madison, Wisconsin

Robert J. Shannon, MSPH
Boston, Massachusetts

Walter E. Stamm, MD
Seattle, Washington

Timothy R. Townsend, MD
Baltimore, Maryland

William M. Valenti, MD
Rochester, New York

James Veazey, MD
Albany, New York

Kathy J. Wydra, RN
Rochester, New York



Executive Editor
Diana S. Wheeler

Assistant Editor
Kathleen J. Norvell

Editorial Assistant
Joyce J. Albert

Associate Publisher
Richard N. Roash

Promotion and Circulation Manager
Peter N. Slack

Advertising Sales Representative
Melissa Warner

Charles B. Slack, Inc.
6900 Grove Road
Thorofare, New Jersey 08086